

NFPA 270
Standard Test
Method for
Measurement of
Smoke Obscuration
Using a Conical
Radiant Source
in a Single
Closed Chamber

1998 Edition



National Fire Protection Association, 1 Batterymarch Park, PO Box 9101, Quincy, MA 02269-9101
An International Codes and Standards Organization

Copyright ©
National Fire Protection Association, Inc.
One Batterymarch Park
Quincy, Massachusetts 02269

IMPORTANT NOTICE ABOUT THIS DOCUMENT

NFPA codes and standards, of which the document contained herein is one, are developed through a consensus standards development process approved by the American National Standards Institute. This process brings together volunteers representing varied viewpoints and interests to achieve consensus on fire and other safety issues. While the NFPA administers the process and establishes rules to promote fairness in the development of consensus, it does not independently test, evaluate, or verify the accuracy of any information or the soundness of any judgments contained in its codes and standards.

The NFPA disclaims liability for any personal injury, property or other damages of any nature whatsoever, whether special, indirect, consequential or compensatory, directly or indirectly resulting from the publication, use of, or reliance on this document. The NFPA also makes no guaranty or warranty as to the accuracy or completeness of any information published herein.

In issuing and making this document available, the NFPA is not undertaking to render professional or other services for or on behalf of any person or entity. Nor is the NFPA undertaking to perform any duty owed by any person or entity to someone else. Anyone using this document should rely on his or her own independent judgment or, as appropriate, seek the advice of a competent professional in determining the exercise of reasonable care in any given circumstances.

The NFPA has no power, nor does it undertake, to police or enforce compliance with the contents of this document. Nor does the NFPA list, certify, test or inspect products, designs, or installations for compliance with this document. Any certification or other statement of compliance with the requirements of this document shall not be attributable to the NFPA and is solely the responsibility of the certifier or maker of the statement.

NOTICES

All questions or other communications relating to this document and all requests for information on NFPA procedures governing its codes and standards development process, including information on the procedures for requesting Formal Interpretations, for proposing Tentative Interim Amendments, and for proposing revisions to NFPA documents during regular revision cycles, should be sent to NFPA headquarters, addressed to the attention of the Secretary, Standards Council, National Fire Protection Association, 1 Batterymarch Park, P.O. Box 9101, Quincy, MA 02269-9101.

Users of this document should be aware that this document may be amended from time to time through the issuance of Tentative Interim Amendments, and that an official NFPA document at any point in time consists of the current edition of the document together with any Tentative Interim Amendments then in effect. In order to determine whether this document is the current edition and whether it has been amended through the issuance of Tentative Interim Amendments, consult appropriate NFPA publications such as the *National Fire Codes*[®] Subscription Service, visit the NFPA website at www.nfpa.org, or contact the NFPA at the address listed above.

A statement, written or oral, that is not processed in accordance with Section 16 of the Regulations Governing Committee Projects shall not be considered the official position of NFPA or any of its Committees and shall not be considered to be, nor be relied upon as, a Formal Interpretation.

The NFPA does not take any position with respect to the validity of any patent rights asserted in connection with any items which are mentioned in or are the subject of this document, and the NFPA disclaims liability of the infringement of any patent resulting from the use of or reliance on this document. Users of this document are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, is entirely their own responsibility.

Users of this document should consult applicable federal, state, and local laws and regulations. NFPA does not, by the publication of this document, intend to urge action that is not in compliance with applicable laws, and this document may not be construed as doing so.

Licensing Policy

This document is copyrighted by the National Fire Protection Association (NFPA). By making this document available for use and adoption by public authorities and others, the NFPA does not waive any rights in copyright to this document.

1. Adoption by Reference – Public authorities and others are urged to reference this document in laws, ordinances, regulations, administrative orders, or similar instruments. Any deletions, additions, and changes desired by the adopting authority must be noted separately. Those using this method are requested to notify the NFPA (Attention: Secretary, Standards Council) in writing of such use. The term “adoption by reference” means the citing of title and publishing information only.

2. Adoption by Transcription – **A.** Public authorities with lawmaking or rule-making powers only, upon written notice to the NFPA (Attention: Secretary, Standards Council), will be granted a royalty-free license to print and republish this document in whole or in part, with changes and additions, if any, noted separately, in laws, ordinances, regulations, administrative orders, or similar instruments having the force of law, provided that: (1) due notice of NFPA’s copyright is contained in each law and in each copy thereof; and (2) that such printing and republication is limited to numbers sufficient to satisfy the jurisdiction’s lawmaking or rule-making process. **B.** Once this NFPA Code or Standard has been adopted into law, all printings of this document by public authorities with lawmaking or rule-making powers or any other persons desiring to reproduce this document or its contents as adopted by the jurisdiction in whole or in part, in any form, upon written request to NFPA (Attention: Secretary, Standards Council), will be granted a nonexclusive license to print, republish, and vend this document in whole or in part, with changes and additions, if any, noted separately, provided that due notice of NFPA’s copyright is contained in each copy. Such license shall be granted only upon agreement to pay NFPA a royalty. This royalty is required to provide funds for the research and development necessary to continue the work of NFPA and its volunteers in continually updating and revising NFPA standards. Under certain circumstances, public authorities with lawmaking or rule-making powers may apply for and may receive a special royalty where the public interest will be served thereby.

3. Scope of License Grant – The terms and conditions set forth above do not extend to the index of this document.

(For further explanation, see the Policy Concerning the Adoption, Printing, and Publication of NFPA Documents, which is available upon request from the NFPA.)

Copyright © 1998 NFPA, All Rights Reserved

NFPA 270

**Standard Test Method for
Measurement of Smoke Obscuration Using a Conical Radiant Source
in a Single Closed Chamber**

1998 Edition

This edition of NFPA 270, *Standard Test Method for Measurement of Smoke Obscuration Using a Conical Radiant Source in a Single Closed Chamber*, was prepared by the Technical Committee on Fire Tests and acted on by the National Fire Protection Association, Inc., at its Annual Meeting held May 18–21, 1998, in Cincinnati, OH. It was issued by the Standards Council on July 16, 1998, with an effective date of August 5, 1998, and supersedes all previous editions.

This edition of NFPA 270 was approved as an American National Standard on August 6, 1998.

Origin and Development of NFPA 270

This standard is based on the 1997 edition of NFPA 258, *Standard Research Test Method for Determining Smoke Generation of Solid Materials*, with minor revisions. Originally the NFPA 258 standard was used for research and as a product development tool. This NFPA 270 standard was developed so that it could be used within the regulatory community for enforcement purposes. This document was developed under a different title and number designation so as not to confuse the end user and in order to establish and clarify the intention and limitations that are now part of the standard.

Technical Committee on Fire Tests

Jesse J. Beitel, *Chair*
Hughes Assoc. Inc., MD [SE]

April L. Berkol, ITT Sheraton Corp., NY [U]
Rep. American Hotel & Motel Assn.

John A. Blair, The DuPont Co., DE [M]
Rep. Society of the Plastics Industry Inc.

William P. Chien, State of New York Dept. of Fire Prevention & Control, NY [E]

William E. Fitch, Omega Point Laboratories Inc., TX [RT]

Sam W. Francis, American Forest & Paper Assn., PA [M]

Thomas W. Fritz, Armstrong World Industries Inc., PA [M]

James R. Griffith, Southwest Research Inst., TX [RT]

Marcelo M. Hirschler, GBH Int'l, CA [SE]

Alfred J. Hogan, Reedy Creek Improvement District, FL [E]

Rep. Fire Marshals Assn. of North America

Karl D. Houser, Gypsum Assn., DC [M]

William E. Koffel, Jr., Koffel Assoc. Inc., MD [SE]

James R. Lawson, U.S. Nat'l Inst. of Standards and Technology, MD [RT]

Gerald E. Lingenfelter, American Ins Services Group Inc., NY [I]

William S. Metes, Underwriters Laboratories Inc., IL [RT]

George E. Meyer, Warnock Hersey, Inc., CA [RT]

John W. Michener, Milliken Research Corp., SC [M]
Rep. American Textile Mfrs. Inst. Inc.

James A. Milke, University of Maryland, MD [SE]

James C. Norris, Union Carbide Corp., TN [M]

John Roberts, Underwriters Laboratories of Canada, ON, Canada [RT]

T. Hugh Talley, Hugh Talley Co., TN [M]

Rep. Upholstered Furniture Action Council

David K. Tanaka, Factory Mutual Research Corp., MA [I]

Richard P. Thornberry, The Code Consortium, Inc., CA [SE]

Robert J. Wills, American Iron & Steel Inst., AL [M]

Peter J. Gore Willse, Industrial Risk Insurers, CT [I]
Rep. Industrial Risk Insurers

Alternates

Delbert F. Boring, Jr., American Iron & Steel Inst., OH [M]
(Alt. to R. J. Wills)

Tony Crimi, Underwriters Laboratories of Canada, ON, Canada [RT]
(Alt. to J. Roberts)

Philip J. DiNenno, Hughes Assoc. Inc., MD [RT]
(Alt. to J. J. Beitel)

Richard G. Gann, U.S. Nat'l Inst. of Standards and Technology, MD [RT]
(Alt. to J. R. Lawson)

Richard D. Gottwald, Society of the Plastics Industry Inc., DC [M]
(Alt. to J. A. Blair)

Marc L. Janssens, Southwest Research Inst., TX [RT]
(Alt. to J. R. Griffith)

Gene V. Paolucci, Yasuda Fire & Marine Insurance Co. of America, NY [I]
(Alt. to G. E. Lingenfelter)

R. Joseph Pearson, Inchcape Testing Services NA Inc., NY [RT]
(Alt. to G. E. Meyer)

William A. Thornberg, Industrial Risk Insurers, CT [I]
(Alt. to P. J. G. Willse)

James J. Urban, Underwriters Laboratories Inc., IL [RT]
(Alt. to W. S. Metes)

Kay M. Villa, American Textile Mfrs. Inst. Inc., DC [M]
(Alt. to J. W. Michener)

Joe Ziolkowski, American Furniture Mfrs. Assoc., NC [M]
(Alt. to T. H. Talley)

Nonvoting

Robert H. Barker, American Fiber Mfrs. Assn., DC [M]
(Alt. to T. L. Jilg)

James F. Hoebel, U.S. Consumer Product Safety Commission, MD [C]

Tod L. Jilg, Hoechst Celanese Corp., NC [M]
Rep. to American Fiber Mfrs. Assn.

Herman H. Spaeth, Novato, CA [C]
(Member Emeritus)

Walter P. Sterling, NFPA Staff Liaison

This list represents the membership at the time the Committee was balloted on the text of this edition. Since that time, changes in membership may have occurred. A key to classifications is found at the back of this document.

NOTE: Membership on a committee shall not in and of itself constitute an endorsement of the Association or any document developed by the committee on which the member serves.

Committee Scope: This Committee shall have primary responsibility for documents on fire testing procedures for reviewing existing fire test standards and recommending appropriate action to NFPA; for recommending the application of and advising on the interpretation of acceptable test standards for fire problems of concern to NFPA technical committees and members; and for acting in a liaison capacity between NFPA and the committees of other organizations writing fire test standards. This Committee does not cover fire tests that are used to evaluate extinguishing agents, devices, or systems.

Contents

Chapter 1 General	270- 4	5-10 Frequency of Checking and Calibrating Procedures.....	270-13
1-1 Scope.....	270- 4	5-11 Total System.....	270-14
1-2 Definitions.....	270- 4	Chapter 6 Conditioning	270-14
1-3 Summary of Test Method.....	270- 4	6-1 Pre-Test.....	270-14
1-4 Significance and Use.....	270- 5	6-2 Conditioning.....	270-14
1-5 Limitations.....	270- 5	Chapter 7 Test Procedure	270-14
Chapter 2 Test Apparatus	270- 5	7-1 Initial Conditions.....	270-14
2-1 General.....	270- 5	7-2 Tests with Pilot Flame.....	270-14
2-2 Test Chamber.....	270- 6	7-3 Preparation of Photometric System.....	270-14
2-3 Sample Support and Heating Arrangements.....	270- 6	7-4 Loading Specimen.....	270-14
2-4 Gas Supply.....	270- 9	7-5 Recording of Light Transmission.....	270-14
2-5 Photometric System.....	270- 9	7-6 Observations.....	270-14
2-6 Chamber Leakage.....	270-10	7-7 Termination of Test.....	270-14
2-7 Cleaning Materials.....	270-10	7-8 Specimen Mass.....	270-15
2-8 Ancillary Equipment.....	270-10	7-9 Repeat Tests.....	270-15
Chapter 3 Test Environment	270-10	Chapter 8 Calculations	270-15
3-1 Light Interference.....	270-10	8-1 Specific Optical Density, D_s	270-15
3-2 Product of Combustion Venting.....	270-10	8-2 Clear Beam Correction Factor, D_c	270-15
3-3 Operator Safety.....	270-10	8-3 Mass Loss.....	270-15
Chapter 4 Test Specimen	270-10	Chapter 9 Test Report	270-15
4-1 Suitability of Sample for Testing.....	270-10	9-1 Descriptive Information.....	270-15
4-2 Sample Face.....	270-10	9-2 Test Results.....	270-16
4-3 Number of Specimens.....	270-11	Chapter 10 Referenced Publications	270-16
4-4 Additional Specimens.....	270-11	Appendix A Explanatory Material	270-16
4-5 Size of Specimens.....	270-11	Appendix B Precision and Bias	270-18
4-6 Specimen Preparation.....	270-11	Appendix C Interlaboratory Application	270-21
4-7 Wrapping of Specimens.....	270-11	Appendix D Determination of Mass Optical Density (MOD)	270-22
Chapter 5 Setup, Calibration, and Maintenance ...	270-11	Appendix E Referenced Publications	270-26
5-1 Setup and Calibration Procedures.....	270-11	Index	270-27
5-2 Alignment of Photometric System.....	270-11		
5-3 Selection of Compensating Filter(s).....	270-12		
5-4 Linearity Check.....	270-12		
5-5 Calibration of Range-Extension Filter.....	270-12		
5-6 Chamber Leakage Rate Test.....	270-13		
5-7 Burner Calibration.....	270-13		
5-8 Radiator Cone Calibration.....	270-13		
5-9 Cleaning.....	270-13		

NFPA 270

Standard Test Method for

Measurement of Smoke Obscuration Using a
Conical Radiant Source in a Single Closed
Chamber

1998 Edition

NOTICE: An asterisk (*) following the number or letter designating a paragraph indicates that explanatory material on the paragraph can be found in Appendix A.

Information on referenced publications can be found in Chapter 10 and Appendix E.

Chapter 1 General

1-1 Scope.

1-1.1 This is a fire-test-response standard.

1-1.2 This test method shall provide a means of measuring smoke obscuration resulting from subjecting essentially flat materials, products, or assemblies (including surface finishes), not exceeding 25 mm in thickness, to specified levels of thermal irradiance, from a conical heater, in a single closed chamber, in the absence or presence of a pilot flame, when placed in a horizontal orientation.

1-1.3 The principal fire-test-response characteristic obtained from this test method is the specific optical density of smoke from the specimens tested, which is obtained as a function of time, for a period of 10 minutes. Other fire-test-response characteristics shall also be permitted to be determined.

1-1.4 An optional fire-test-response characteristic measurable with this test method is the mass optical density, which is the specific optical density of smoke divided by the mass lost by the specimens during the test.

1-1.5 This test method is based on ISO 5659-2, *Determination of Specific Optical Density by a Single-Chamber Test*, and provides equivalent results to ISO 5659-2.

1-1.6 The fire-test-response characteristics obtained from this test are specific to the specimen tested, in the form and thickness tested, and are not an inherent property of the material, product, or assembly.

1-1.7 This test method does not provide information on the fire performance of the test specimens under fire conditions other than those conditions specified in this test method. For limitations of this test method, see Section 1-5.

1-1.8 The values stated in SI units shall be considered the required values. The values given in parentheses are for information only.

1-1.9 This standard measures and describes the response of materials, products, or assemblies to heat and flame under controlled conditions, but does not by itself incorporate all factors required for fire hazard or fire risk assessment of the materials, products, or assemblies under actual fire conditions.

1-1.10 Fire testing of products and materials is inherently hazardous, and adequate safeguards for personnel and property

shall be employed in conducting these tests. This test method is known to involve hazardous materials, operations, and equipment. (See also 2-2.2, 2-2.3, and 7-7.2.)

1-1.11 This standard does not purport to address all of the safety problems, if any, associated with its use. It shall be the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.

1-2 Definitions. For definitions of terms used in this test method, refer to the terminology contained in ASTM E 176, *Terminology of Fire Standards*, and ISO 3261, *Fire Tests — Vocabulary*.

Assembly. A unit or structure composed of a combination of materials or products, or both.

Composite. A combination of materials that are generally recognized as distinct entities — for example, coated or laminated materials.

Continuous (as related to data acquisition). Conducted at data collection intervals of 5 seconds or less.

Exposed Surface. That surface of the specimen subjected to the incident heat.

Ignition. The initiation of combustion evidenced by glow, flame, detonation, or explosion, either sustained or transient.

Mass Optical Density (MOD). The ratio of the optical density of smoke and the mass loss of the test specimen, multiplied by the volume of the test chamber and divided by the length of the light path.

Sample. An amount of the material, product, or assembly to be tested that is representative of the item as a whole.

Smoke Obscuration. Reduction in visibility due to smoke.

Specimen. The actual section of material, product, or assembly to be placed in the test apparatus.

Shall. Indicates a mandatory requirement.

Time to Ignition. Time between the start of the test and the presence of a flame on or over most of the specimen surface for a period of at least 4 seconds.

1-3 Summary of Test Method.

1-3.1 This test method shall employ a conically shaped, electrically heated radiant energy source, contained within a stainless steel tube, and positioned so as to produce an irradiance level of up to 50 kW/m², averaged over the center of the exposed surface of an essentially flat specimen, mounted horizontally, to determine smoke obscuration inside a closed chamber. The actual irradiance levels used for standard testing shall be 25 kW/m² and 50 kW/m².

1-3.2 The specimen shall be 75 mm × 75 mm at a thickness not exceeding 25 mm and shall be mounted horizontally within a holder.

1-3.3 The exposure shall be conducted in the absence or in the presence of a pilot flame. (See 2-3.6.) If the pilot flame is present, the test shall be deemed to be in the “flaming” mode; if it is absent, the test shall be deemed to be in the “nonflaming” mode.

1-3.4 The test specimens shall be exposed to nonflaming or flaming conditions within a closed chamber. A photometric system with a vertical light path shall be used to measure the varying light transmission as smoke accumulates. The light

transmittance measurements shall be used to calculate the specific optical density of the smoke generated during the test.

1-3.5 The specimens shall be exposed to two conditions, out of the four standard exposure conditions, to be chosen by the test requester. The four standard exposure conditions shall be as follows:

- (a) Flaming at an irradiance of 25 kW/m²
- (b) Flaming at an irradiance of 50 kW/m²
- (c) Nonflaming at an irradiance of 25 kW/m²
- (d) Nonflaming at an irradiance of 50 kW/m²

The default conditions for testing, unless specified otherwise, shall be those in the flaming mode. Exposures to other irradiances shall also be possible.

1-3.6* Mass optical density shall be an optional fire-test-response characteristic obtainable from this test method by using a load cell that continuously monitors the mass of the test specimen.

1-4 Significance and Use.

1-4.1* This test method shall provide a means for determining the specific optical density of the smoke generated by specimens of materials, products, or assemblies under the specified exposure conditions. Values determined by this test shall be specific to the specimen in the form and thickness tested and shall not be inherent fundamental properties of the material, product, or assembly tested. Therefore, closely repeatable or reproducible experimental results shall not be expected from this test method when tests are conducted for a given material, product, or assembly, while introducing variations in properties such as specimen thickness or density.

1-4.2* Physiological aspects associated with vision shall not be measured by this method.

1-4.3* Predicting the smoke obscuration to be generated by the specimens upon exposure to heat or flame under any fire conditions other than those specified shall not be permitted.

1-5 Limitations.

1-5.1 The following behavior during a test shall render that test invalid:

- (a) Self-ignition in the nonflaming mode
- (b) A specimen being displaced from the zone of controlled irradiance so as to touch the pilot burner or the pilot flame
- (c) Extinction of the pilot flame (even for a short period of time) in the flaming mode
- (d) Molten material overflowing the specimen holder

1-5.2* Evaluation of the data obtained, together with the individual masses, shall assist in assessing the reasons for any observed variability in measurements.

1-5.3* The results of the test shall apply only to the thickness of the sample as tested.

1-5.4 Sensitivity to variations requires that when changing to another sample to be tested, it shall first be necessary to clean and remove from the walls all accumulated residues to ensure that chemical or physical recombination with the effluents or residues produced as a result of the thermal irradiance does not affect the data obtained. Even when testing the same sample, excessive accumulations of residue shall not be permitted

to build up, since ruggedness tests have indicated that such deposits serve as additional insulators, tending to reduce normally expected condensation of the aerosol, thereby raising the measured specific optical density.

1-5.5* In this procedure, the specimens shall be subjected to one or more specific sets of laboratory test conditions. If different test conditions are substituted or the end-use conditions are changed, it shall not necessarily be possible by or from this test method to predict changes in the fire-test-response characteristics measured. Therefore, the results shall be valid only for the fire test exposure conditions described in this procedure.

1-5.6* Information relating the specific optical density obtained by this test method to the mass lost by the specimen during the test shall be possible only by using the (optional) load cell to determine the mass optical density.

1-5.7* This test method does not use dynamic measurements. Therefore, the smoke obscuration values obtained shall not represent conditions of open fires.

Chapter 2 Test Apparatus

2-1 General. The apparatus shall consist of an airtight test chamber with provision for containing a sample holder, radiation cone, pilot burner, light transmission and measuring system, and other ancillary facilities for controlling the conditions of operation during a test. (See Figure 2-1.)

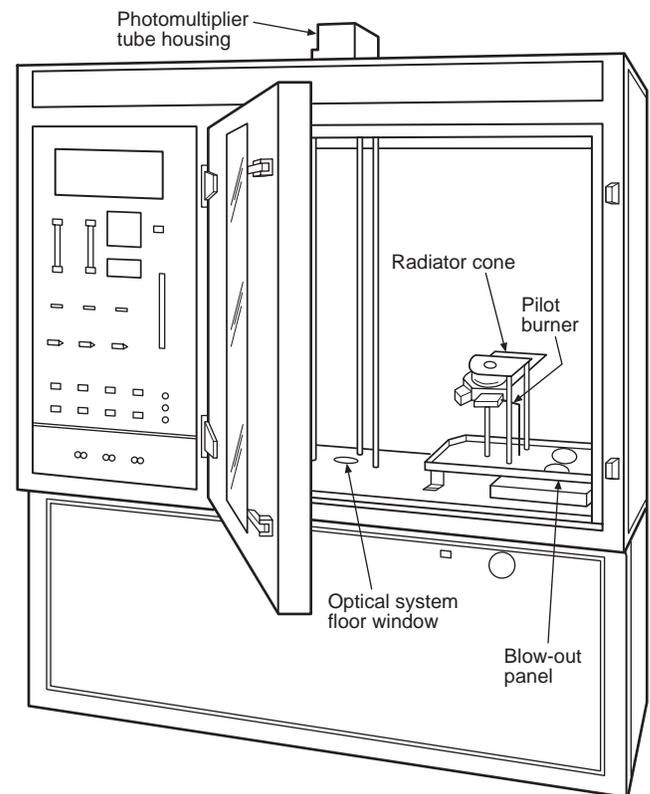


Figure 2-1 Typical arrangement of test chamber.

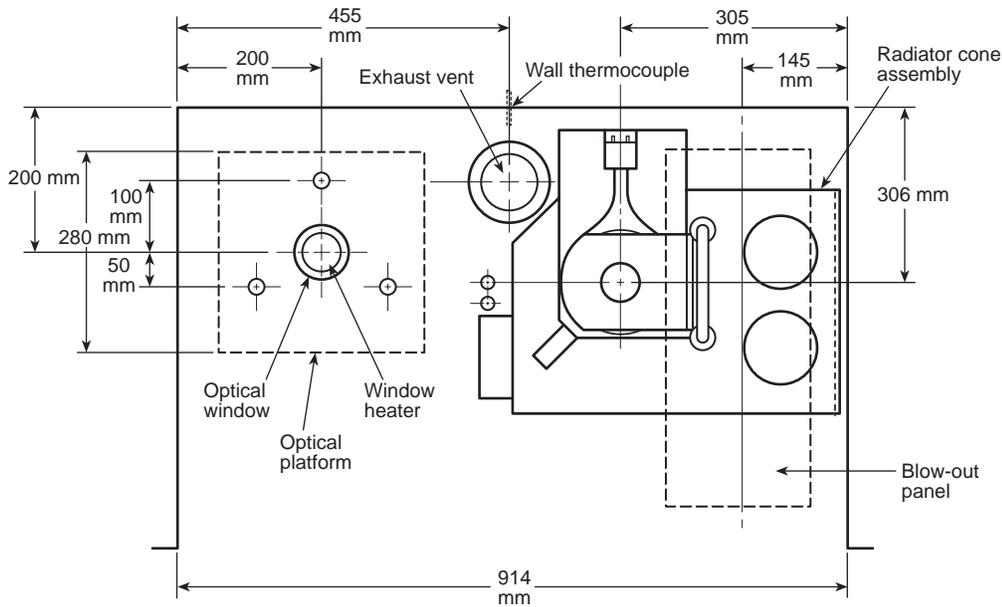


Figure 2-2.1 Plan view of typical test chamber.

2-2 Test Chamber.

2-2.1 The test chamber shall be fabricated from laminated panels, the inner surfaces of which shall consist of either a porcelain-enameled metal, not more than 1 mm thick, or an equivalent coated metal, which is resistant to chemical attack and corrosion and capable of easy cleaning. (See Figures 2-1 and 2-2.1.) The internal dimensions of the chamber shall be $914 \text{ mm} \pm 3 \text{ mm}$ long, $914 \text{ mm} \pm 3 \text{ mm}$ high, and $610 \text{ mm} \pm 3 \text{ mm}$ deep. (See Figure 2-2.1.) The chamber shall be provided with a hinged front-mounted door with an observation window and a removable opaque door cover to the window to prevent light entering the chamber.

2-2.2* A safety blow-out panel consisting of a sheet of aluminum foil of thickness not greater than 0.04 mm and having a minimum area of $80,600 \text{ mm}^2$ shall be provided in the chamber, fastened in such a way as to provide an airtight seal.

2-2.3 Two optical windows, each with a diameter of $75 \text{ mm} \pm 1 \text{ mm}$, shall be mounted, one each in the top and bottom of the cabinet, at the position shown in Figure 2-2.1, with their interior faces flush with the outside of the cabinet lining. The underside of the window on the floor shall be provided with an electric heater of approximately 9 W capacity, in the form of a ring, which shall be capable of maintaining the upper surface of the window at a temperature just sufficient to minimize smoke condensation on that face (a temperature of 50°C to 55°C has been found suitable) and shall be mounted around its edge so as not to interrupt the light path. Optical platforms, $8 \text{ mm} \pm 0.1 \text{ mm}$ thick, shall be mounted around the windows on the outside of the chamber and shall be held rigidly in position relative to each other by three metal rods, each with a diameter of at least 12.5 mm, extending through the chamber and fastened securely to the platforms.

2-2.4 Other openings in the cabinet shall be provided for services, as specified and where appropriate. They shall be capable of being closed so that a positive pressure up to 1.5 kPa above atmospheric pressure can be developed inside the chamber (see 2-2.6) and maintained when checked in accordance with Sections 2-6 and 5-6. All components of the chamber shall be capable of withstanding a greater internal positive pressure than the safety blow-out panel.

2-2.5 An inlet vent with a shutter shall be provided in the front of the chamber at the top and away from the radiator cone, and an exhaust vent with a shutter shall be provided in the bottom of the chamber to lead, via flexible pipe with a diameter of 50 mm to 100 mm, to an extraction fan capable of creating a negative pressure of at least 0.5 kPa.

2-2.6* Chamber Pressure Control Facilities. Provision shall be made for controlling the pressure inside the test chamber. A water manometer, with a range of up to 1.5 kPa, shall be provided for connection to a pressure regulator and to a tube in the top of the chamber.

2-2.7 A thermocouple measuring junction made from wires of a diameter not greater than 1 mm shall be mounted on the inside of the back wall of the chamber, at the geometric center, by means of an insulating disc (such as polystyrene foam) that has a thickness of $6.5 \text{ mm} \pm 0.2 \text{ mm}$ and a diameter of not more than 20 mm attached with a suitable cement. The thermocouple junction shall be connected to a recorder, meter, or data acquisition unit, and the system shall be suitable for measuring temperatures in the range of 35°C to 60°C . (See 7-1.3.)

2-3 Sample Support and Heating Arrangements.

2-3.1 Radiator Cone.

2-3.1.1 The radiator cone (see Figure 2-3.1.1) shall consist of a heating element of nominal rating 450 W contained within a stainless steel tube, $2210 \text{ mm} \pm 5 \text{ mm}$ in length and $6.5 \text{ mm} \pm 0.2 \text{ mm}$ in diameter, coiled into the shape of a truncated cone

and fitted into a shade. The shade shall have an overall height of $45 \text{ mm} \pm 0.04 \text{ mm}$, an internal diameter of $55 \text{ mm} \pm 1 \text{ mm}$, and an internal base diameter of $110 \text{ mm} \pm 3 \text{ mm}$. It shall consist of two layers of $1 \text{ mm} \pm 0.1 \text{ mm}$ thick stainless steel with a $10 \text{ mm} \pm 0.5 \text{ mm}$ thickness of ceramic fiber insulation of nominal density 100 kg/m^3 sandwiched between them. The heating element shall be clamped by two plates at the top and bottom of the element.

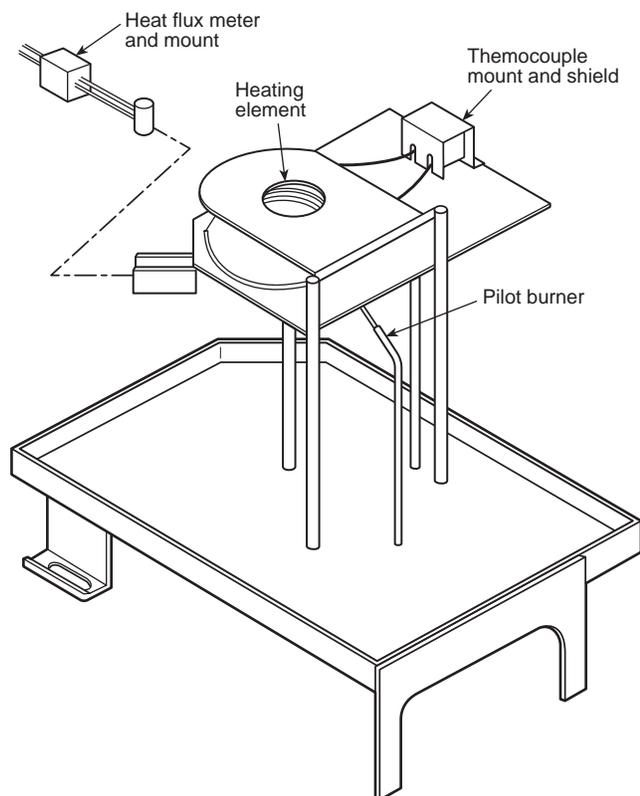


Figure 2-3.1.1 Typical framework for support of radiator cone, specimen holder, and flux meter.

2-3.1.2 The radiator cone shall be capable of providing irradiance in the range of 10 to 50 kW/m^2 , at the center of the surface of the specimen. When the irradiance is determined at two other positions, $25 \text{ mm} \pm 2 \text{ mm}$ each side of the specimen center, the irradiance at these two positions shall be not less than 85 percent, or not more than 115 percent of the irradiance at the center of the specimen.

2-3.1.3* The irradiance of the radiator cone shall be controlled by reference to the averaged reading of two Type K thermocouples. The thermocouples shall have a $1.6 \text{ mm} \pm 0.2 \text{ mm}$ outside diameter, sheathed with an unexposed hot junction, mounted diametrically opposite, in contact with, but not welded to the heating element, and positioned at one-third of the distance from the top surface of the cone.

2-3.1.4* The temperature at the heater shall be controlled and shall be held steady to $\pm 2^\circ\text{C}$. The temperature controller for the radiator cone shall be of the proportional, integral, and derivative type 3-term controller with thyristor stack fast-cycle or phase angle control of not less than 10-A maximum rating. Capacity for adjustment of integral time between 10

seconds and 50 seconds and differential time between 25 seconds and 30 seconds shall be provided to permit reasonable matching with the response characteristics of the heater. A temperature input range of 0°C to 1000°C shall be suitable. Automatic cold junction compensation of the thermocouple shall be provided. Alternate devices that give equivalent results shall be permitted to be accepted.

2-3.2 Framework for Radiator Cone. The radiator cone shall be secured from the vertical rods of the support framework and shall be located so that the lower rim of the radiator cone shade is $25 \text{ mm} \pm 1 \text{ mm}$ above the upper surface of the specimen when oriented in the horizontal position [see Figures 2-3.2(a) and 2-3.2(b)]. The base of the specimen holder shall contain a height adjustment device to ensure a consistent distance between radiator cone and specimen surface.

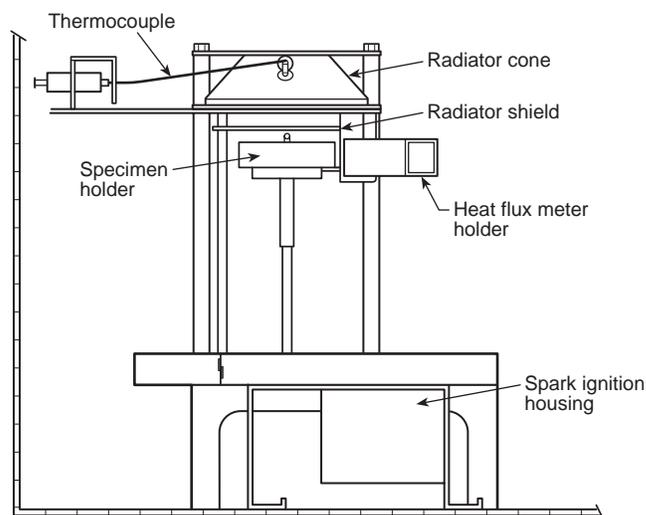


Figure 2-3.2(a) Typical arrangement of radiator cone, specimen holder, and radiation shield (side view).

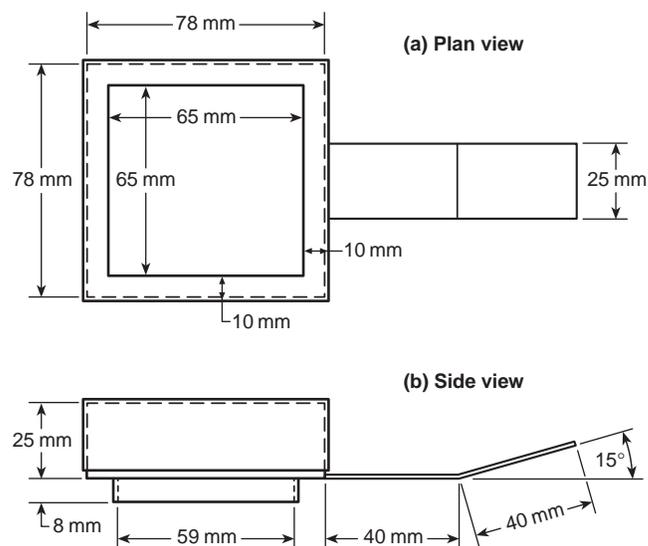


Figure 2-3.2(b) Specimen holder.

2-3.3 Radiation Shield.

2-3.3.1 The cone heater shall be provided with a removable radiation shield to protect the specimen from the irradiance prior to the start of the test. The radiation shield shall be made of noncombustible material with a total thickness not to exceed 12 mm. The radiation shield shall comply with one of the following:

- (a) A water-cooled radiation shield coated with a durable matte black finish of surface emissivity, $\epsilon = 0.95 \pm 0.05$
- (b) A radiation shield with a reflective top surface in order to minimize radiation transfer, but not water cooled

2-3.3.2* The radiation shield shall be equipped with a handle or other suitable means for quick insertion and removal. The cone heater base plate shall be equipped with the means for holding the radiation shield in position and allowing its easy and quick removal.

2-3.4 Heat Flux Meter.

2-3.4.1* The heat flux meter shall be of the foil (Gardon) or thermopile (Schmidt-Boelter) type with a design range of at least 50 kW/m^2 . The target receiving the radiation shall have a flat, circular face of $10 \text{ mm} \pm 1 \text{ mm}$ diameter, coated with a durable matte black finish. [See Figure 2-3.2(a).] The target shall be water cooled.

2-3.4.2* The heat flux meter shall be connected directly to a suitable recorder or data acquisition unit, so that it is capable, when calibrated, of recording heat fluxes of 25 kW/m^2 and 50 kW/m^2 to an accuracy of $\pm 1 \text{ kW/m}^2$

2-3.4.3 The heat flux meter system shall be calibrated by comparing its response with that of a primary reference standard, when exposed to irradiances of 25 kW/m^2 and $50 \text{ kW/m}^2 \pm 1 \text{ kW/m}^2$, averaged over the $10 \text{ mm} \pm 1 \text{ mm}$ diameter area of the heat flux meter. (See Section B-1.)

2-3.5 Specimen Holders.

2-3.5.1 The specimen holder base shall be lined with a low-density (nominal 65 kg/m^3) refractory fiber blanket, with a minimum thickness of 10 mm. (See Figure 2-3.5.1.)

2-3.5.2* A retainer frame and wire grid shall be used for all tests. The wire grid shall be $75 \text{ mm} \pm 1 \text{ mm}$ square with $20 \text{ mm} \pm 0.5 \text{ mm}$ square holes constructed from $2 \text{ mm} \pm 0.2 \text{ mm}$ stainless steel rod welded at all intersections.

2-3.6* Pilot Burner. The flame from the single-flame burner shall have a length of $30 \text{ mm} \pm 5 \text{ mm}$ and shall be positioned horizontally $10 \text{ mm} \pm 1 \text{ mm}$ above the top face of the specimen. [See Figures 2-3.6(a) and 2-3.6(b).] The color of the flame shall be blue with a yellow tip. The tip of the burner shall reach the edge of the specimen itself. [See Figure 2-3.6(b).]

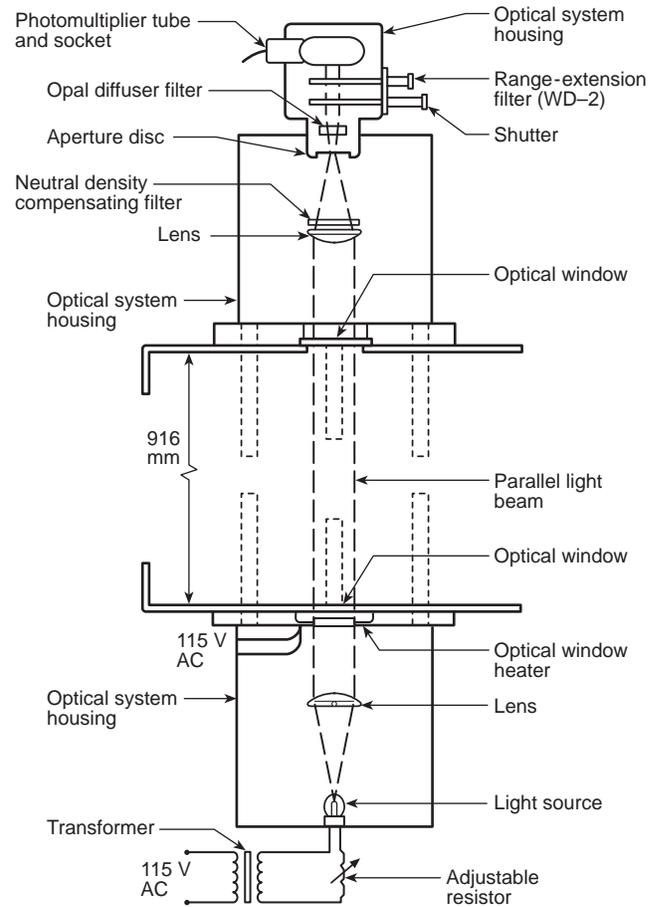


Figure 2-3.5.1 Photometric system.

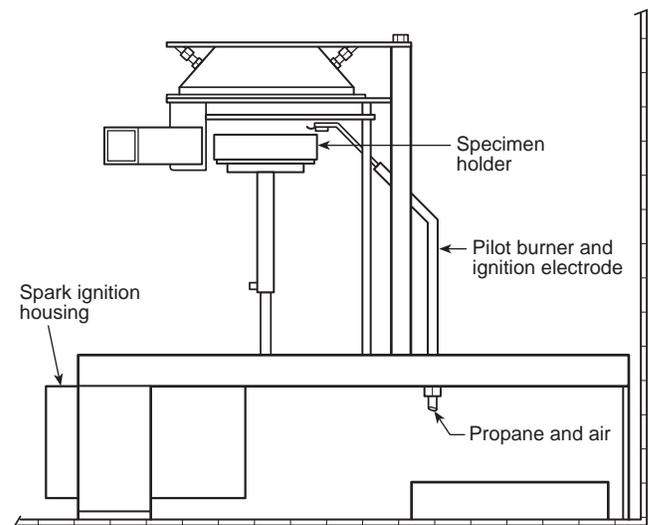


Figure 2-3.6(a) Typical arrangement of radiator cone, specimen holder, and radiation shield (front view).

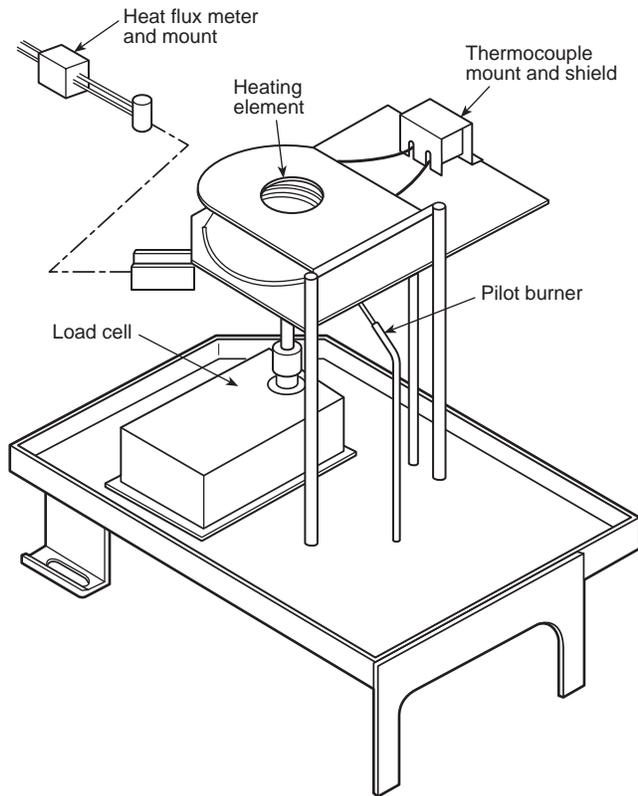


Figure 2-3.6(b) Typical framework for support of radiator cone, specimen, and flux meter.

2-4 Gas Supply. A mixture of propane of at least 95 percent purity and at a pressure of $3.5 \text{ kPa} \pm 1 \text{ kPa}$ and air at a pressure of $170 \text{ kPa} \pm 30 \text{ kPa}$ shall be supplied to the burner. Each gas shall be fed to the point at which they are mixed and supplied to the burner. The use of needle valves and calibrated flowmeters shall be a suitable method of controlling gas flows. The flowmeter for the propane supply shall be capable of measuring $50 \text{ cm}^3/\text{min}$ flow rates and that for air a value of $500 \text{ cm}^3/\text{min}$. Alternate devices shown to give equivalent results also shall be acceptable.

2-5 Photometric System.

2-5.1 General.

2-5.1.1 The photometric system shall consist of a light source and lens in a lighttight housing mounted below the optical window in the floor of the cabinet and a photodetector with lens, filters, and a shutter in a lighttight housing above the optical window in the top of the chamber.

2-5.1.2 The system shall be as shown in Figure 2-5.1.2. Equipment shall be provided to control the output of the light source and to measure the amount of light falling on the photodetector.

2-5.2 Light Source. The light source shall be a 6.5-V incandescent lamp. Power for the lamp shall be provided by a transformer producing 6.5 V and a rheostat so that the voltage across the lamp, as determined by an ac voltmeter, is main-

tained at $4 \text{ V} \pm 0.2 \text{ V rms}$. The lamp shall be mounted in the lower lighttight box, and a lens to provide a collimated light beam of 51 mm diameter, passing toward and through the optical window on the floor of the chamber, shall be mounted, with provision for adjustment, to control the collimated beam in direction and diameter. The housing shall be provided with a cover to allow access for adjustments to be made to the position of the lens.

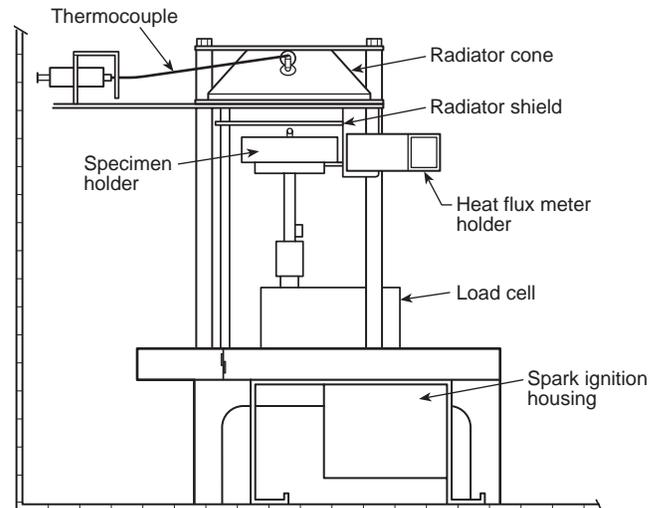


Figure 2-5.1.2 Typical arrangement of radiator cone, specimen holder, and radiator shield (side view) with load cell for mass optical density determination.

2-5.3 Photodetector.

2-5.3.1* The light-measuring device system shall consist of a photomultiplier tube connected to a multirange amplifier coupled to a recording device or data acquisition unit (see 2-8.6). This system shall be capable of continuously measuring relative light intensity against time as percentage transmission over at least five orders of magnitude, with an S-4 spectral sensitivity response similar to that of human vision and a dark current less than 10^9 A . The system shall have a linear response with respect to transmittance and an accuracy of better than ± 3 percent of the maximum reading on any range. For selection of photomultiplier tubes, as applicable, the minimum sensitivity shall allow a 100 percent reading to be obtained with a 0.5 neutral density filter and an ND-2 range-extension filter (see 2-5.3.2) in the light path. Provision shall be made for adjusting the reading of the instrument under given conditions over the full range of any scale.

2-5.3.2 The photomultiplier tube shall be mounted in the upper section of the detector housing. Below the tube there shall be an assembly that provides for the rapid positioning of a filter and of a shutter, in or out of the path of the collimated light beam, each being operated separately. The filter, referred to as the range-extension filter (ND-2), shall be a glass neutral density filter of nominal optical density 2. When in the closed position, the shutter shall prevent all light in the test chamber from reaching the photomultiplier tube. An opal diffuser shall be permanently mounted below the shutter.

2-5.3.3 The lower part of the housing shall support a 51 mm \pm 1 mm diameter lens, capable of being adjusted so that the collimated beam is focused to form a small intense spot of light at the disc aperture between the upper and lower parts of the housing. Above the lens, there shall be a mount for supporting one or more compensating filters from a set of nine gelatin neutral density filters, with optical density varying from 0.1 to 0.9 in increments of 0.1. The housing shall be provided with a cover to allow access for making adjustments to the position of the lens and for inserting or removing filters.

2-5.3.4* A neutral density filter, with a nominal optical density of 3.0, large enough to cover the lower optical window, the actual optical density having been determined by calibration, shall be available for calibrating the photometric system.

2-5.4 Additional Equipment.

2-5.4.1 A template for checking the collimated light beam shall consist of an opaque disc marked with a concentric ring of 51 mm \pm 1 mm diameter, and shall be capable of fitting snugly between the support pillars. It shall be capable of being attached to, and centered on, the underside of the upper optical window in the chamber.

2-5.4.2 A piece of white cloth, paper tissue, or a neutral density filter of sufficient size to completely cover the lower optical window of the chamber and that is capable of transmitting a sufficient amount of light to give a midscale reading of the photometric system when switched to the scale with a range of 1 percent transmission shall be available for calibrating the range-extender filter.

2-5.4.3 A piece of opaque material sufficiently large enough to cover the lower optical window shall be available for blocking the light from the light source entering the chamber.

2-6* Chamber Leakage. With the specified items of equipment properly assembled and ready for test, the chamber shall be sufficiently airtight to comply with the requirements of the leakage rate test given in Section 5-6.

2-7* Cleaning Materials. The optical system windows, viewing window, chamber walls, and specimen holders shall be cleaned regularly.

2-7.1* Optical System Windows. The exposed surfaces of the glass separating the photodetector and light-source housings from the interior of the chamber shall be cleaned after each test.

2-7.2 Viewing Window. The viewing window shall be cleaned to allow the chamber interior to be viewed during testing.

2-7.3* Chamber Walls. The chamber walls shall be cleaned periodically to prevent excessive build-up of smoke products.

2-7.4 Specimen Holders. Remove any charred residues on the specimen holders and horizontal rods securing the holder position to prevent contamination of subsequent specimens.

2-8 Ancillary Equipment.

2-8.1 Balance. The balance shall have a capacity exceeding the mass of the specimen and shall be readable and accurate to 0.5 percent of the specimen mass.

2-8.2 Timing Device. A timing device capable of recording elapsed time to the nearest second, over a period of at least 1 hour, with an accuracy of 1 second in 1 hour, shall be used for timing operations and observations.

2-8.3 Linear Measuring Devices. Rules, calipers, gauges, or other devices of suitable accuracy shall be used for checking all dimensions specified with given tolerances.

2-8.4 Auxiliary Heater. An auxiliary heater of 500 W capacity, capable of raising the air temperature uniformly without local heating of the walls, shall be permitted to be used, if required, to help the chamber to reach the stabilized temperature more rapidly under adverse conditions.

2-8.5 Protective Equipment. Protective clothing, such as gloves, goggles, and respirators, and handling equipment, such as tongs, shall always be available and shall be used when the type of sample being tested demands them.

2-8.6 Data Acquisition. A recorder, or data acquisition unit, shall be available and shall be capable of continuously recording the millivolt output of the photodetector to an accuracy of better than 0.5 percent of full range deflection. (*See 2-5.3.*) The device used shall also be capable of recording the heat flux meter output to the required accuracy. (*See 2-3.4.2.*) If a data acquisition unit is used, the data collection intervals shall be 5 seconds or less. If a recorder is used, the recording chart drive shall be used at a minimum chart speed of 10 mm/min.

2-8.7* Thermometer. A thermometer, or a Type K thermocouple, shall be available and shall be capable of measuring temperature over the range 20°C to 100°C to an accuracy of $\pm 0.5^\circ\text{C}$.

2-8.8 Water Circulating Device. A device for water circulation shall be provided to cool the heat flux meter.

Chapter 3 Test Environment

3-1 Light Interference. The test apparatus shall be protected from direct sunlight, or any strong light source, to avoid the possibility of spurious light readings.

3-2 Product of Combustion Venting. Adequate provision shall be made for removing potentially hazardous and objectionable smoke and gases from the area of operation. Suitable precautions shall be taken to prevent exposure of the operator to such gases, particularly during the removal of specimens from the chamber or when cleaning the apparatus.

3-3* Operator Safety. The operator shall use heavy gloves, safety tongs, or other suitable protection for removal of the specimen holder. The venting shall be checked periodically for proper operation.

Chapter 4 Test Specimen

4-1 Suitability of Sample for Testing.

4-1.1 The method shall be intended for essentially flat samples only. Essentially flat surfaces shall be those where the irregularity from a plane does not exceed ± 1 mm.

4-1.2 The results of this test method shall be sensitive to variations in surface characteristics, thickness of individual layers, overall thickness, mass, and composition.

4-2 Sample Face. If the two faces of samples submitted for evaluation by this method are different, both faces shall be evaluated if it is possible that both faces are exposed to fire when in use.

4-3* Number of Specimens. A minimum of six specimens shall be tested, so that three specimens are tested at each one of the two required conditions. Unless otherwise specified by the test requester, the standard exposure conditions shall be as follows:

- (a) Flaming at an irradiance of 25 kW/m²
- (b) Flaming at an irradiance of 50 kW/m²

4-4 Additional Specimens.

4-4.1 An additional number of specimens, as specified in Section 4-3, shall be used for each face in accordance with the requirements of Section 4-2.

4-4.2 An additional nine specimens (three specimens per mode to be tested) shall be held in reserve, in case they are required by the conditions specified in 7-9.2.

4-5 Size of Specimens.

4-5.1 The specimens shall be square with sides 75 mm.

4-5.2* Thickness.

4-5.2.1 Whenever possible, test samples shall be in their end-use thickness. Samples used with a thickness of 25 mm or less shall be evaluated at their full thickness.

4-5.2.2 If no information on sample thickness is available, materials shall be permitted to be tested at a thickness of 1.0 mm, unless otherwise specified in the material or performance standard or specification.

4-5.2.3 Samples with a thickness greater than 25 mm shall be cut to give a specimen thickness of 25 mm, in such a way that the original (uncut) face is evaluated.

4-5.2.4 Samples of multilayer materials, products, or assemblies with a thickness greater than 25 mm, consisting of core material(s) with facings of different materials, shall be prepared according to 4-5.2.3. (*See also 4-6.2.*)

4-6 Specimen Preparation.

4-6.1 The specimen shall be representative of the material, product, or assembly, and shall be prepared in accordance with the procedures described in 4-6.2 and 4-6.3. The specimens shall be cut, sawn, molded, or stamped from identical sample areas of the material, product, or assembly, and records shall be kept of their thicknesses and, if required, their masses.

4-6.2 If flat sections of the same thickness and composition are tested in place of curved, molded, or specialty parts, this shall be stated in the test report. Any substrate or core materials for the specimens shall be the same as those used in practice.

4-6.3 When coatings, including paints and adhesives, are tested with the substrate or core as used in practice, specimens shall be prepared following normal practice and in such cases the method of application of the coating, number of coats, and type of substrate shall be included in the test report.

4-7 Wrapping of Specimens.

4-7.1 All specimens shall be covered across the back, along the edges, and over the front surface periphery leaving a central exposed specimen area of 65 mm \pm 5 mm \times 65 mm \pm 5 mm, with a single sheet of aluminum foil that is 0.04 mm \pm 0.005 mm thick with the dull side in contact with the specimen. Care shall be taken not to puncture the foil or to intro-

duce unnecessary wrinkles during the wrapping operation. The foil shall be folded so as to minimize losses of any molten material at the bottom of the holder. After mounting the specimen into its holder, any excess foil along the front edges shall be trimmed off, as appropriate.

4-7.2 All wrapped specimens shall be backed with one or more sheets of noncombustible insulating board of an oven dry density of 850 kg/m³ \pm 100 kg/m³ and a nominal thickness of 12.5 mm to ensure that the top edges of the specimen are pressed against the retaining lips of the specimen holder. Wrapped specimens less than 25 mm thick shall be backed with at least one sheet of noncombustible board with or without a layer of mineral fiber blanket underneath to accommodate a wider variety of specimen thicknesses.

4-7.3 In the case of resilient materials, products, or assemblies, each specimen shall be installed in its aluminum foil wrapper, in the holder, in such a way that the exposed surface lies flush with the inside face of the opening of the specimen holder. Specimens with uneven exposed surfaces shall not protrude beyond the plane of the opening of the specimen holder.

4-7.4 When thin impermeable specimens, such as thermoplastic films, swell during the test due to gases trapped between the film and the backing, they shall be maintained essentially flat by making two or three cuts (20 mm to 40 mm long) in the film, to act as vents.

Chapter 5 Setup, Calibration, and Maintenance

5-1 Setup and Calibration Procedures.

5-1.1* The apparatus shall be assembled, connected to the services and control devices as specified in Chapter 6, and checked for the proper functioning of the various systems, including the electrical connections, to ensure good electrical contact.

5-2 Alignment of Photometric System.

5-2.1 General. The setup procedure shall be conducted as detailed in 5-2.2 and 5-2.3 in the initial setup of the apparatus, after the replacement of the light source or after the occurrence of some accidental misalignment. The procedure for selecting the appropriate compensating filter(s) shall be followed after each setup procedure. (*See Section 5-3.*)

5-2.2 Beam Collimation.

5-2.2.1 The optical platforms shall be checked for rigidity. The opaque-disc template shall be attached to the lower face of the upper optical window with the marked ring downwards and centered on the window. The light source shall be switched on and its projected image adjusted on the template so that the light beam completely fills the 51-mm diameter ring with no more light outside the ring than is necessary to satisfy this requirement.

5-2.2.2* Adjustments shall be made by removing the cover to the light source enclosure, releasing the lower lens mount fixings, and repositioning the lens mount so that the light pattern on the template is centered and of the correct size.

5-2.2.3* The lens mount shall be reattached and the cover replaced, ensuring that the test cabinet has been adequately resealed. The template shall be removed from the upper optical window.

5-2.3 Beam Focusing. The cover to the housing on top of the test chamber shall be opened, the compensating filter holder shall be removed, and the lens mount shall be slackened. With the photodetector system switched off and the light source switched on, the lens mount shall be adjusted for focusing and alignment so that the converging beam forms a small intense spot of light on the aperture to the photomultiplier tube housing. The lens mount shall be tightened, the beam focusing adjustment shall be checked, the compensating filter holder shall be replaced, and the enclosure cover shall be closed and sealed.

5-3* Selection of Compensating Filter(s). The faces of both optical windows inside the test chamber shall be cleaned. The photometric system shall be switched on with the range-extension filter in the light path, the shutter open, and the multi-range meter set to the range capable of recording 100 percent light transmission. The control for adjusting the reading of the instrument to determine whether a reading of 100 percent is achievable shall be operated. If it is, no change in the compensating filter shall be required; if not, another compensating filter shall be used to satisfy this requirement.

5-4 Linearity Check.

5-4.1 The photometric system shall be switched on with the range-extension filter in the light path and the shutter closed. The zeroing device shall be adjusted to give a reading of 0 percent transmission with the instrument range switched to a full-scale reading of 100 percent transmission; the instrument shall be switched to the other ranges to determine that the recorded transmission remains 0 percent.

5-4.2 The calibrated filter, with a nominal optical density of 3.0, shall be placed in the light path over the lower optical window, the shutter shall be opened, and the percentage of transmission shall be measured. The difference between the observed reading and the calibrated value, when expressed as a percentage of the average of the two values, shall be within 5 percent.

5-5 Calibration of Range-Extension Filter. The apparatus shall be brought to its normal operating condition (*see Section 7-1*) with the chamber wall temperature remaining steady at $40^{\circ}\text{C} \pm 5^{\circ}\text{C}$. The photometric system with the range-extension filter in the light path and with the shutter open shall be switched on, and the amplifier shall be switched to its 100 percent transmission range. The white cloth, sheets of tissue, or filter with an optical density of about 2.5 shall be placed over the lower optical window and the amplifier switched to the 1 percent transmission range. (*See 2-5.3.*) The reading shall be set to 0.50 percent by adjusting the instrument. Without disturbing the cloth, tissue, or filter, reset the amplifier to the 100 percent transmission, and the range-extension filter, ND-2, shall be withdrawn from the light path. The transmission reading, T_s , shall be recorded and used to determine the value of the appropriate correction factor, C_f , for readings obtained when the range-extension filter is not in the light path. (*See Table 5-5.*)

Exception: For materials, products, or assemblies having known performance, this calibration procedure shall not be needed unless the optical density is greater than 3.

Table 5-5 Correction Factors with Neutral Density Filter (ND-2) Removed

Meter Indication T_s	Correction Factor C_f	Optical Density of Neutral Density Filter
31	-27.4	1.79
32	-25.6	1.81
33	-23.8	1.82
34	-22.1	1.83
35	-20.4	1.845
36	-18.8	1.86
37	-17.3	1.87
38	-15.7	1.88
39	-14.2	1.89
40	-12.8	1.90
41	-11.4	1.91
42	-10.0	1.92
43	-8.6	1.93
44	-7.3	1.94
45	-6.0	1.95
46	-4.8	1.96
47	-3.5	1.97
48	-2.3	1.98
49	-1.2	1.99
50	0.0	2.00
51	+1.1	2.01
52	+2.2	2.02
53	+3.3	2.025
54	+4.4	2.03
55	+5.5	2.04
56	+6.5	2.05
57	+7.5	2.06
58	+8.5	2.064
59	+9.5	2.07
60	+10.5	2.08
61	+11.4	2.086
62	+12.3	2.09
63	+13.2	2.10
64	+14.2	2.107
65	+15.0	2.114
66	+15.9	2.12
67	+16.8	2.13
68	+17.6	2.135
69	+18.5	2.14
70	+19.3	2.146

5-6 Chamber Leakage Rate Test. The airtightness of the test chamber shall be measured on each occasion of use (with the door, vents, and spare gas sampling pipes closed) by introducing compressed air into the test chamber through one of the gas sampling pipes (or other compressed air inlet) until the pressure recorded on the manometer is over 0.76 kPa and then shutting off the supply. The airtightness of the test chamber shall be such that the time taken for the recorded pressure to drop from 0.76 kPa to 0.50 kPa, as determined by using the timing device, shall be not less than 5.0 minutes.

5-7 Burner Calibration. Set the propane flow to 88.5 cm³/min ± 1.0 cm³/min and the airflow to 270 cm³/min ± 20 cm³/min. (See Section 2-4.)

5-8 Radiator Cone Calibration.

5-8.1 The apparatus shall be cleaned of any residues left from previous tests and, when a cone calibration is to follow soon after a test, the chamber shall be flushed with air for 2 minutes (with the door shut and the exhaust and inlet vents open). The heat flux meter shall be mounted as specified in 2-3.2 and shall be connected to the electrical and water services.

5-8.2 The burner shall not be ignited during this calibration. The apparatus shall be brought to its normal operating condition (see Section 7-1), with the chamber wall temperature remaining steady (see 7-1.3), and the radiation shield moved away from the cone.

5-8.3* With the chamber door closed, the inlet vent open, and the exhaust vent closed, water shall be supplied to the heat flux meter to cool the heat flux meter body. The heat flux

meter output shall be monitored to determine when thermal equilibrium has been reached. The cone shall then be adjusted, as necessary, to give a steady millivolt reading corresponding to the calibrated value equivalent to an irradiance of 25 kW/m², or 50 kW/m², as required. If the door is opened for any reason during calibration, sufficient time shall be allowed after closing the door for thermal equilibrium to be reached before taking the final millivolt reading.

5-8.4 The procedure in 5-8.3 shall be repeated as necessary to calibrate the equipment in three positions — at the center and at 25 mm ± 1 mm on each side of the center.

5-8.5 Radiation Shield.

5-8.5.1 The radiation shield shall be returned to the position below the cone, and the heat flux meter shall be removed from the test chamber so that tests on specimens can proceed immediately.

5-8.5.2 Water shall be circulated through the heat flux meter until the meter is cool enough for the protective cap to be replaced without melting or distortion.

5-9* Cleaning. The inside walls of the chamber and the supporting framework for the cone and specimen holders shall be cleaned using materials as described in Section 2-7, whenever periodic visual inspection indicates the need.

5-10 Frequency of Checking and Calibrating Procedures.

5-10.1* Regular checking and calibration shall be undertaken in accordance with Table 5-10.1.

Table 5-10.1 Frequency of Checks and Calibrations

Item of Equipment	Maximum Interval Between Checks and Calibrations	Procedure (Section Reference)
Test chamber interior	Before testing every specimen and before any calibration	5-9
Radiator cone	Once every test day and when renewed or replaced	5-8
Chamber leakage rate	Once every test day and when new seals or safety blow-out panel are fitted	5-6
Heat flux meter	Every 3 months and when cleaned or recoated	2-3.4.3
Photometric system:		
Calibration	Before testing every specimen	7-3
Alignment	Every 6 months and when light source is replaced or when damage is incurred	5-2
Compensating filters	Every 6 months and when transmission through windows deteriorates	5-3
Linearity	Every 6 months and when transmission through windows deteriorates	5-4
Range-extension filter	Every 6 months	5-5
Total system	Every month, or after the system has been used for more than 100 tests	5-11

5-10.2 The relevant setup procedure shall be followed after any part of the equipment has been renewed or repaired.

5-11* Total System. The total system shall be checked by testing a material or product with repeatable results. A record of the test results shall be maintained; if erratic values are observed, any instrumental or operational deficiencies shall be identified and corrected.

Chapter 6 Conditioning

6-1 Pre-Test. Prior to testing, the specimens shall be conditioned to constant mass in an atmosphere at a temperature of $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$ and a relative humidity of 50 ± 10 percent. Constant mass shall be considered to have been reached when two successive weighing operations, carried out at an interval of 24 hours, do not differ by more than 0.1 percent of the mass of the test piece, or 0.1 g, whichever is greater. The specimen shall be tested within 10 minutes of removal from the conditioning atmosphere, if the test room conditions differ from the above.

6-2* Conditioning. While in the conditioning chamber, specimens shall be supported in racks, so that air has access to all surfaces.

Chapter 7 Test Procedure

7-1 Initial Conditions.

7-1.1 The mass of each test specimen, wrapped in aluminum foil, shall be recorded before placing it inside the specimen holder, to generate an initial mass, m_i (in grams).

7-1.2 The test chamber shall be prepared according to the requirements of Chapter 5, with the radiator cone set at an irradiance of 25 kW/m^2 or 50 kW/m^2 .

7-1.3* If a test has just been completed, the test chamber shall be flushed with air with the test chamber door closed and the exhaust and inlet vents open, until it is completely clear of smoke. The inside of the cabinet shall be inspected and the walls and the supporting framework shall be cleaned wherever necessary (see Section 5-9). The faces of the optical windows inside the chamber shall be cleaned before each test. The apparatus shall be allowed to stabilize until the chamber wall temperature is within the range of $40^{\circ}\text{C} \pm 5^{\circ}\text{C}$ for tests with the radiator cone at 25 kW/m^2 or within the range $55^{\circ}\text{C} \pm 5^{\circ}\text{C}$ for tests with the radiator cone at 50 kW/m^2 . The inlet valve shall be closed.

7-2 Tests with Pilot Flame.

7-2.1 For tests with the pilot flame, with the burner in its correct position, the gas and air supplies shall be turned on and the burner shall be ignited. Then, the flow rates shall be checked and, if necessary, adjusted to ensure that they are in accordance with Section 5-7.

7-2.2 If the pilot flame is extinguished by gaseous effluent during a test and fails to reignite within 10 seconds, the gas supply to the pilot burner shall be switched off immediately.

7-3 Preparation of Photometric System. The photometric system shall be prepared as follows:

- (a) Set the recorder to zero and then open the shutter to set the full scale 100 percent transmission reading.

- (b) Close the shutters and check and reset the zero, if necessary, using the most sensitive 0.1 percent range.
- (c) Recheck the 100 percent setting.
- (d) Repeat the sequence of operations until accurate 100 percent and zero readings are obtained on the amplifier and recorder, or data acquisition unit, when the shutters are opened and closed.

7-4 Loading Specimen.

7-4.1 A wrapped specimen, prepared in accordance with Sections 4-3 and 4-4 with its insulating board as noted in 4-7.2, shall be placed in its holder. The holder and specimen shall be placed on the supporting framework below the radiator cone and the test chamber door shall be closed immediately.

7-4.2 The test shall be started by removing the radiation shield from below the cone and simultaneously starting the recording chart drive or data acquisition unit and closing the inlet vent.

7-4.3 If preliminary tests indicate that the pilot flame is extinguished before the radiation shield is removed, then it shall be necessary to remedy this problem with the equipment before continuing with the test.

7-5 Recording of Light Transmission.

7-5.1 The percentage of light transmission and the corresponding time shall be recorded continuously from the start of the test (which corresponds to the time when the radiation shield was removed). The range of the photodetector amplifier system shall be switched to the next decade when required so that readings less than 10 percent of full-scale deflection are avoided.

7-5.2 If the light transmission falls below 0.01 percent, the observation window in the chamber door shall be covered and the range-extension filter shall be withdrawn from the light path.

7-6* Observations. Any particular burning characteristics of the specimens, such as delamination, intumescence, shrinkage, melting, dripping, collapse, occurrence of pool fire under the test specimen, or any other event of special interest, shall be recorded and the time at which the particular behavior occurs, including the time to ignition and duration of flaming, also shall be recorded. The smoke characteristics, such as color, and the nature of the settled particulate matter also shall be recorded. All times shall be reported from the moment the test was started. (See 7-4.2.)

7-7 Termination of Test.

7-7.1 The test shall be conducted for a period of 10 minutes. This test shall be permitted to be conducted for periods in excess of 10 minutes when minimum light transmittance values have not been reached during a 10-minute exposure. If the period exceeds 10 minutes, the test time shall be reported.

7-7.2* The burner shall be extinguished if the pilot flame has been used.

7-7.3 The radiation shield shall be moved below the cone.

7-7.4 The exhaust fan shall be switched on and, when the water manometer indicates a small negative pressure, the inlet vent shall be opened and shall continue exhausting until a maximum value of light transmission is recorded, with the appropriate range selected, and noted as the "clear beam"

reading, T_c , for use in correcting for deposits on the optical windows.

7-8 Specimen Mass. At the conclusion of each test, the final specimen mass, m_f (in grams), shall be determined after removal from the specimen holder. The aluminum foil in which the specimen had been wrapped during the test for determining the mass shall be included.

7-9 Repeat Tests.

7-9.1 The percentage of light transmission of two sets of three specimens for each sample, one set for each mode from among the four standard exposure conditions shown below, shall be measured. The default exposure conditions, unless specified otherwise by the test requester, shall be those with a pilot flame.

- Mode 1: Irradiance — 25 kW/m² with pilot flame
- Mode 2: Irradiance — 50 kW/m² with pilot flame
- Mode 3: Irradiance — 25 kW/m² without pilot flame
- Mode 4: Irradiance — 50 kW/m² without pilot flame

7-9.2* If during a test, one or more of the three replicate specimens show any of the following behaviors, an additional specimen of the identical preconditioned sample shall be tested in the test mode in which the unusual behavior(s) occurred.

- (a) Self-ignition in the nonflaming mode
- (b) A specimen being displaced from the zone of controlled irradiance so as to touch the pilot burner or the pilot flame
- (c) Extinction of the pilot flame (even for a short period of time) in the flaming mode

Exception: The test results of a specimen that does not cease flaming after the pilot flame goes out, shall not be considered valid.

- (d) Molten material overflowing the specimen holder

A maximum of six specimens shall be allowed to be tested. Data obtained from the improper tests noted above shall not be incorporated in the averaged data but the occurrence shall be reported. The test method shall not be suitable if three or more of the specimens tested show any of the above characteristics.

7-9.3 For each individual specimen, the percentage value of light transmission shall be determined and, from this, the appropriate specific optical density shall be calculated, as given in Chapter 8. If the value of D_s at 10 minutes for an individual specimen differs from the average value for the set of three specimens of which it is part by more than 50 percent of that average for no apparent reason, an additional set of three specimens shall be tested from the same sample in the same mode, and the average of all six results obtained shall be recorded.

Chapter 8 Calculations

8-1 Specific Optical Density, D_s ,

8-1.1 For each specimen, the set of continuous recorded data of light transmission against time shall be used and the results at 1.5 minutes, 4.0 minutes, and 10.0 minutes shall be converted to specific optical density, D_s , by using the following equation, where $T\%$ is a value of the percent light transmittance, taken from the continuous record.

$$D_s = 132 \log_{10} \frac{100}{T\%}$$

The factor 132 shall be derived from the physical characteristics of the chamber by using the following equation:

$$\frac{V}{A \times L} = 132$$

where:

V = volume of the chamber

A = exposed area of the specimen

L = length of the light path

8-1.2 A correction factor, C_f , shall be added to the value of D_s , as determined in 8-1.1. This correction factor shall depend upon the use of the range-extension filter. The value of C_f shall be zero if one of the following applies.

- (a) The filter is in the light path at the time the transmission was recorded ($T\% \geq 0.01\%$).
- (b) The photometric system is not equipped with a removable filter.
- (c) The ND-2 filter is of the correct optical density of 2.

The value of C_f shall be as determined by the procedure described in Section 5-5 (and Table 5-5) if the filter is moved out of the light path at the time it is measured ($T\% < 0.01\%$).

8-2 Clear Beam Correction Factor, D_c . For each specimen, the value of the "clear beam" reading, T_c , shall be recorded to determine the correction factor D_c . (See 7-7.4.) D_c shall be calculated as for D_s in Section 8-1. The correction factor D_c shall not be required to be recorded if it is less than 5 percent of the maximum specific optical density as determined from that which is created by plotting the recording of light versus time in Sections 8-1 and 9-2(c). (See Section 8-1.)

8-3* Mass Loss. For each valid specimen tested, the total mass loss, D_m (in grams), shall be calculated and recorded using the following equation:

$$D_m = m_1 - m_2$$

where:

m_1 = initial mass of the specimen (including the aluminum foil used for testing) (in grams)

m_2 = mass of the specimen after the test (with all the foil wrappings included) (in grams)

Chapter 9 Test Report

9-1 Descriptive Information. The following descriptive information shall be included in the test report:

- (a) Name and address of the testing laboratory
- (b) Date and identification number of the report
- (c) Name and address of the test requester, when applicable
- (d) Name of manufacturer or supplier of material, product, or assembly tested, if known
- (e) Commercial name or other identification marks and description of the sample
- (f) Full description of the sample, including such details as type, form, essential dimension, mass or density, color, and coverage rate of any coating

- (g) Full description of specimen construction and preparation (*see Sections 4-5 and 4-6*)
- (h) Face of specimen tested (*see Sections 4-5 and 4-6*)
- (i) Thickness of each specimen tested
- (j) Conditioning of the test specimens
- (k) Date of the test
- (l) Modes of testing, indicating irradiance and use of the pilot flame for each specimen
- (m) Number of specimens tested for each type of exposure
- (n) Test number and any special remarks

9-2 Test Results. The following test results shall be included in the test report:

- (a) Table of numerical results containing the following information for each valid specimen tested:
 1. Specific optical density at 1.5 minutes
 2. Specific optical density at 4.0 minutes
 3. Specific optical density at 10.0 minutes
 4. Specific optical density at end of test (if test duration is different from 10.0 minutes)
 5. Maximum specific optical density
 6. Time to ignition
 7. Time to maximum optical density
 8. Duration of the test
 9. If calculated, the neutral density correction, C_f
 10. The clear beam correction factor, D_c
 11. The mass loss, D_m
- (b) Graphical results, for each valid specimen tested
- (c) Graph of specific optical density against time
- (d) All available information required in Section 4-7 (regarding specimen preparation and coatings used, if applicable) and in Section 7-6 (observations regarding burning characteristics of the specimens and any events of special interest during the tests)
- (e) Details of any invalid tests, including reasons for them being invalid (*See 1-5.1 and 7-9.2.*)

Chapter 10 Referenced Publications

10-1 The following documents or portions thereof are referenced within this standard as mandatory requirements and shall be considered part of the requirements of this standard. The edition indicated for each referenced mandatory document is the current edition as of the date of the NFPA issuance of this standard. Some of these mandatory documents might also be referenced in this standard for specific informational purposes and, therefore, are also listed in Appendix E.

10-1.1 ASTM Publication. American Society for Testing and Materials, 100 Barr Harbor Drive, West Conshohocken, PA 19428-2959.

ASTM E 176-97a, *Terminology of Fire Standards*, 1997.

10-1.2 ISO Publications. ISO Central Secretariat 1, rue de Varembé Case postale 56 CH-1211 Genève 20 Switzerland.

ISO 5659-2, *Determination of Specific Optical Density by a Single Chamber Test*, 1994.

ISO 3261, *Fire Tests — Vocabulary*, 1975.

Appendix A Explanatory Material

Appendix A is not a part of the requirements of this NFPA document but is included for informational purposes only. This appendix contains explanatory material, numbered to correspond with the applicable text paragraphs.

A-1-3.6 See Appendix D for additional information on mass optical density.

A-1-4.1 The current smoke density chamber test, NFPA 258, *Standard Research Test Method for Determining Smoke Generation of Solid Materials* (ASTM E 662, *Test Method for Specific Optical Density of Smoke Generated by Solid Materials*), is used in the United States by specifiers of floor coverings and in the rail transportation industries. The measurement of smoke obscuration is important to the researcher and the product development scientist. This test method, which incorporates improvements over ASTM E 662, will also increase the usefulness of smoke obscuration measurements to the specifier and to product manufacturers.

A-1-4.2 The photometric scale used to measure smoke by this test method is similar to the optical density scale for human vision. As with many smoke obscuration test methods, correlation with measurements by other test methods has not been established.

A-1-4.3 At the present time no basis exists for predicting the smoke obscuration by specimens not exposed to the specified fire conditions.

A-1-5.2 Results obtained from this test method have proven to be affected by small variations in sample geometry, surface orientation, thickness (either overall or individual layer), mass, and composition. It is, therefore, critical that the replicate samples be cut, sawed, or blanked to identical sample areas, and that records be kept of the respective masses with the individual test data.

Preselection of samples with identical thickness or mass, or both, will reduce the variability but is not necessarily truly indicative of the actual variability to be expected from the sample as normally supplied.

A-1-5.3 There is no simple mathematical formula applicable to calculate the specific optical density of a thickness of sample different from that tested. Some information on a relationship between optical density and thickness is found in Grand 1976.

Results obtained from this test method are affected by small variations of the position of the sample and radiometer relative to the radiant heat source.

A-1-5.5 The measurements obtained have also proven sensitive to small differences in conditioning (*see Chapter 5*). Many materials, products, or assemblies, such as carpeting and thick sections of wood, plastics, or plywood, require long periods to attain equilibrium (constant weight) even in a forced-draft conditioning chamber.

This test method solves some of the limitations associated with other closed chamber test methods, such as NFPA 258, *Standard Research Test Method for Determining Smoke Generation of Solid Materials* and ASTM E 662, *Test Method for Specific Optical Density of Smoke Release Rates for Materials and Products* (Breden, Meisters 1976; Babrauskas 1981; Quintiere 1982), but some additional limitations remain.

A-1-5.6 The atmosphere inside the chamber during some tests becomes oxygen-deficient before the end of the experi-

ment, and combustion often ceases when the oxygen concentration decreases. Therefore, for heavy composites, for example, it is possible that the layers farthest away from the radiant source will not undergo combustion. Walls cause losses of combustion particulates through deposition. (See Appendix D for additional information.)

A-1-5.7 Soot and other solid or liquid combustion products settle on the optical surfaces during a test, resulting in potentially higher smoke density measurements than those caused by the smoke in suspension.

A-2-2.2 Stainless steel wire mesh offers adequate protection for the blow-out panel.

A-2-2.6 A suitable pressure regulator should consist of an open water-filled bottle and a length of flexible tubing inserted 100 mm (4 in.) below the water surface; the other end of the tubing should be connected to the manometer and the chamber. (See Figure A-2-2.6.) The regulator should be vented to the exhaust system.

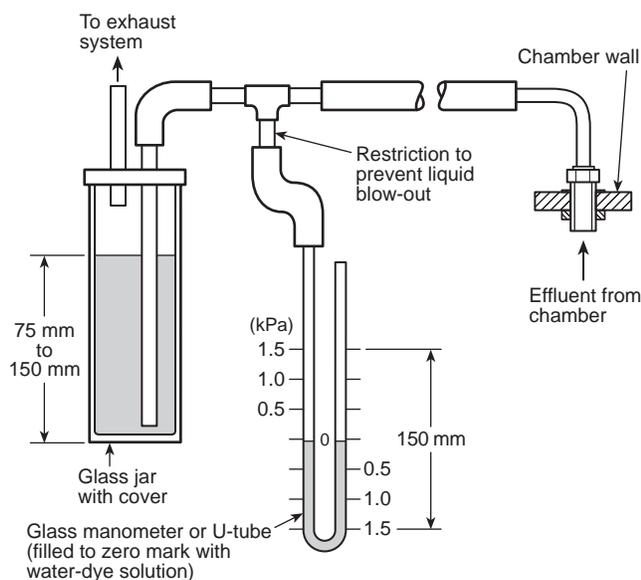


Figure A-2-2.6 Typical chamber pressure relief monometer.

A-2-3.1.3 It has been found that thermocouples of equal length and wired in parallel to the temperature controller perform adequately; alternate wiring methods shown to give equivalent results are also acceptable. Sheathed chromel/alumel Type K thermocouples have been found suitable for this purpose.

A-2-3.1.4 An irradiance of 50 kW/m² will be given by a heater temperature in the 700°C to 750°C temperature range.

While phase angle control is allowed for the temperature controller of the radiator cone, it should be noted that this will usually require electrical filtering to avoid the risk of inducing noise in low signal level lines.

A-2-3.3.2 The radiation shield handle is necessary in order to enable repeat tests to be carried out without switching off the radiator cone.

A-2-3.4.1 The manufacturer of Schmidt-Boelter gauges has the following specifications for cooling water: pressure 413621

kPa, temperature 20.0°C–26.6°C and flow rate 0.76 L/min–1.14 L/min.

A-2-3.4.2 If a recorder that only displays an mV output is used, the mV value should be converted to heat flux, in kW/m², using the calibration factor (or equation, if appropriate) specific to the heat flux meter.

A-2-3.5.2 The retainer frame and wire grid are particularly appropriate when testing intumescent specimens and also for reducing unrepresentative edge combustion of composite samples, or for retaining specimens prone to delamination. The wire grid is likely to affect the test results, compared to tests conducted in its absence. However, its use is recommended for several reasons — it helps to promote uniformity in testing by different laboratories; in view of the expected effect of the retainer frame and wire grid on test results as explained above, it is needed for certain specimens; and it is required in ISO 5659-2.

A-2-3.6 It is recommended that a small spark ignition device be sited next to the outlet tube of the burner, allowing the operator to ignite the flame without opening the door of the chamber. A suitable system is a spark plug with a 3-mm gap powered from a 10-kV transformer. A suitable transformer is of a type specifically designed for spark-ignition use, with an isolated (ungrounded) secondary to minimize interference with the data-transmission lines. An acceptable electrode length and spark plug location is such that the spark gap is located 13 mm above the specimen, close to the pilot burner.

A-2-5.3.1 The required accuracy of the photodetector is obtained more easily if the measuring systems incorporate scale ranges of 30, 3, 0.3, and so on, as well as ranges of 100, 10, 1, and so on.

A-2-5.3.4 Handle all filters by their edges because fingerprints greatly affect their rating. Do not attempt to clean the surface of a filter; once the surface has been damaged, replace the filter.

A-2-6 The most likely sources of leakage have been found to be the door seal, the inlet and outlet vents, and the safety blow-out panel.

A-2-7 Periodic cleaning is essential for proper operation. Appropriate materials for cleaning the inside of the chamber should be made available.

A-2-7.1 Clean the top window first, then the bottom window, using a nonabrasive cloth dampened with a suitable cleaner. Ethyl alcohol, ethyl ketone, or the equivalent, and soft tissue have been found effective for cleaning the optical windows and the viewing window. Dry the window to prevent streaking or film buildup. Do not use any cleaners that contain wax because wax will cause the smoke to be adsorbed to the glass more quickly.

A-2-7.3 An ammoniated spray detergent and soft scouring pads have been found effective for cleaning the chamber walls.

A-2-8.7 The thermometer is intended for determining ambient temperature or any other needed temperature.

A-3-3 The test procedure involves high temperatures and combustion processes. Therefore, it is possible for eye injuries, burns, ignition of extraneous objects, and inhalation of smoke or combustion products to occur, unless proper precautions are taken. To avoid accidental leakage of toxic combustion

products into the surrounding atmosphere, it is advisable to evacuate the chamber, at the end of a test, into an exhaust system with adequate capacity.

A-4-3 Optional testing modes include the following:

- (a) Nonflaming at an irradiance of 25 kW/m² (for comparison with the test results from ASTM E 662)
- (b) Nonflaming at an irradiance of 50 kW/m² (for comparison with the test results from ISO 5659-2)

These exposures are not required. Other testing modes are also possible with this equipment.

A-4-5.2 All specimens consume oxygen when they are combusted in the chamber and the smoke generation of some specimens (especially those undergoing rapid combustion) is influenced by the reduced oxygen concentration in the chamber.

A-5-1.1 Heat up the radiator cone gradually from cold, and do not allow it to overheat or to remain operating without a blank specimen holder — that is, a holder with a specimen in it or the heat flux meter in position in front of it.

A-5-2.2.2 In cases of severe maladjustment, the lamp socket should be repositioned also.

A-5-2.2.3 On occasion this adjustment also includes the optimization of the lens mount position so that the reading given by the photodetector is a maximum. This operation will require removal of the template and should be followed by a final check on the position of the image as described in 5-2.2.3.

A-5-3 An indication of the appropriate filter, or combination of filters, is obtained conveniently by removing any compensating filter in the housing above the test chamber, closing the housing cover, placing a compensating filter(s) over the lower optical window inside the test chamber, and checking the instrument reading. The choice of compensating filter determined this way needs to be confirmed by the specified procedure.

A-5-8.3 With some water circulators it is necessary to have the chamber door slightly open to allow access for the tubing. Allow at least 10 minutes for stabilizing between adjustments.

A-5-9 Because the test is sensitive to variations in the composition of samples, it is desirable to clean the apparatus when changing from tests on one material, product, or assembly to another so that the results are not affected by chemical or physical interaction between the specimen and the residues left from previous tests on products. Even when testing specimens of the same material, product, or assembly, accumulations of residue reduce the amount of deposition of smoke, resulting in an increase in the measured value of specific optical density.

A-5-10.1 Products of combustion of some materials, products, or assemblies might cause corrosion of the cone heating element. This can be compensated for by adjusting the applied voltage for a limited amount of change. If the cone cannot be made to give the required output, a new heating element might be required.

A-5-11 The material should be one that is, and is likely to continue to be, consistently available to the testing laboratory.

A-6-2 Forced-air movement in the conditioning chamber is acceptable to assist in accelerating the conditioning process. The results obtained from this method are sensitive to small differences in specimen conditioning. It is important, therefore, to ensure that the requirements of Sections 6-1 and 6-2 are followed carefully.

A-7-1.3 If the temperature is too high, use of the exhaust fan to draw in cooler air from the laboratory is an adequate procedure.

A-7-6 The smoke generation from some materials, products, or assemblies differs significantly depending on whether combustion occurs in a nonflaming or flaming mode. It is important, therefore, to record as much information as possible about the mode of combustion (for example the presence of flame on the sample surface) during each test.

Coated and faced samples, including sheet laminates, tiles, fabrics, and other composites secured to a substrate with an adhesive, and composites not attached to a substrate, are subject to delamination, cracking, peeling, or other separations affecting their smoke generation.

A-7-7.2 The burner is extinguished in order to reduce the likelihood that the air added during venting will create an explosive mixture in the chamber.

A-7-9.2 If a thin specimen that had not been cut (*see 4-7.4*) swells out of the plane, the results from that specimen should be ignored and an extra cut specimen tested.

A-8-3 Note that the deposition of smoke particulates on walls and lens is one of the reasons that if two materials reach the same peak optical density at different times within the test they are likely to exhibit different fire performance in terms of smoke obscuration, and possibly in terms of mass optical density.

Appendix B Precision and Bias

This appendix is not a part of the requirements of this NFPA document but is included for informational purposes only.

B-1 Precision. Tables B-1(a) and B-1(b) contain information on repeatability and reproducibility, based on a preliminary international interlaboratory evaluation in which batches of sixteen materials were tested in accordance with this test method by eight laboratories in six countries, for plastic materials [*Table B-1(a)*] and building materials [*Table B-1(b)*]. Additional information on repeatability on two wood samples in a single laboratory is presented in Table B-1(c), and repeatability information from another laboratory, which tested six building products, is shown in Table B-1(d). Overall, the results of these preliminary studies indicate that the average coefficient of variability (*CV*) for repeatability is 14.4, while the average coefficient of variability for reproducibility in the international study is 49.0. Results from a more definitive precision study will be made available after a round-robin evaluation has been completed.

B-2 Bias. The bias of this test method is unknown.

Table B-1(a) Repeatabilities and Reproducibilities of Specific Optical Density for Some Plastics

Material	Thickness, mm	Irradiance, kW/m ²	Mean, D _s (10)	Repeatability (within laboratories)		Reproducibility (between laboratories)	
				r	Percent of mean	R	Percent of mean
PMMA	1.0	25	11	4	38	10	91
		25 + pf	55	13	24	29	53
		50	54	11	20	17	32
ABS	1.1	25	312	77	25	311	100
		25 + pf	441	146	33	205	46
		50	435	102	23	192	44
Polyurethane rigid foam (28 kg/m ³)	25.0	25	49	16	32	61	124
		25 + pf	48	24	51	26	54
		50	145	48	33	97	67
Polyurethane flexi- ble foam (27 kg/m ³)	25.0	25	178	49	27	114	64
		25 + pf	80	28	35	56	70
		50	127	46	36	80	63
Expanded polysty- rene (nonfire retardant; 14 kg/m ³)	25.0	25	112	75	67	196	175
		25 + pf	102	75	74	130	128
		50	270	88	33	195	72

Note: pf indicates test carried out with pilot flame.

Table B-1(b) Repeatabilities and Reproducibilities of Specific Optical Density for Some Building Materials

Material	Thickness, mm	Irradiance, kW/m ²	Mean, D _s (10)	Repeatability (within laboratories)		Reproducibility (between laboratories)	
				r	Percent of mean	R	Percent
Pine	12.1	25	403	97	24	300	74
		25 + pf	26	15	55	56	322
		50	196	191	98	191	98
Chipboard	12.2	25	411	47	12	187	45
		25 + pf	58	59	102	88	153
		50	481	96	20	464	97
Plywood	4.2	25	251	31	12	132	52
		25 + pf	33	15	47	58	175
		50	113	58	31	82	72
Medium Density fibreboard	11.9	25	420	127	30	281	67
		25 + pf	68	42	62	72	106
		50	688	114	17	413	60
Paper-faced plasterboard	12.7	25	20	8	42	21	107
		25 + pf	8	8	104	25	314
		50	17	11	64	23	132

Note: pf indicates test carried out with pilot flame.

Table B-1(c) Repeatability Experiments Using Wood Samples in a Single Laboratory

Material	Douglas Fir Plywood	Red Oak Flooring
<i>Incident Flux: 25 kW/m², NF</i>		
D_m (AVG)	496	475
D_m (STD)	47	9
D_m (CV%)	9	2
D_m /g (mass loss) (AVG)	24.2	22.1
D_m /g (mass loss) (STD)	4.7	7.3
D_m /g (mass loss) (CV%)	20	33
<i>Incident Flux: 35 kW/m², NF</i>		
D_m (AVG)	475	461
D_m (STD)	11	12
D_m (CV%)	2	3
D_m /g (mass loss) (AVG)	19.9	11.9
D_m /g (mass loss) (STD)	3.4	2.7
D_m /g (mass loss) (CV%)	17	23
<i>Incident Flux: 40 kW/m², NF</i>		
D_m (AVG)	491	461
D_m (STD)	13	22
D_m (CV%)	3	5
D_m /g (mass loss) (AVG)	22.3	13.4
D_m /g (mass loss) (STD)	4.5	6.0
D_m /g (mass loss) (CV%)	20	45
<i>Overall Statistics</i>		
D_m (AVG)	487	466
D_m (STD)	29	16
D_m (CV%)	6	3
D_m /g (mass loss) (AVG)	22.1	15.8
D_m /g (mass loss) (STD)	4.1	7.1
D_m /g (mass loss) (CV%)	19	45

Note: AVG (average); STD (standard deviation); CV% (coefficient of variance).

Table B-1(d) Repeatability Using Products in a Single Laboratory

Material	E Foam*	Sh Fl 1*	Fl Tle*	PP Crp*	Lens*	Sh Fl 2*
<i>25kW/m², NF</i>						
D_m (AVG)	134	266	178	543	333	483
D_m (STD)	8	9	9	15	17	93
D_m (CV%)	6	3	5	3	5	19
D_{10} (AVG)	111	264	170	521	202	396
D_{10} (STD)	5	9	13	12	25	33
D_{10} (CV%)	5	4	8	2	12	8

Table B-1(d) Repeatability Using Products in a Single Laboratory, Continued

Material	E Foam*	Sh Fl 1*	Fl Tile*	PP Crp*	Lens*	Sh Fl 2*
<i>25 kW/m², F</i>						
<i>D_m (AVG)</i>	29	143	97	340	94	476
<i>D_m (STD)</i>	6	8	37	29	6	20
<i>D_m (CV%)</i>	19	6	38	9	7	4
<i>D₁₀ (AVG)</i>	25	121	91	269	72	344
<i>D₁₀ (STD)</i>	4	7	37	17	5	15
<i>D₁₀ (CV%)</i>	15	6	40	6	7	4
<i>50 kW/m², F</i>						
<i>D_m (AVG)</i>	125	304	144	388	110	691
<i>D_m (STD)</i>	7	15	10	31	8	37
<i>D_m (CV%)</i>	6	5	7	8	2	5
<i>D₁₀ (AVG)</i>	90	205	118	245	77	418
<i>D₁₀ (STD)</i>	5	9	9	20	7	15
<i>D₁₀ (CV%)</i>	5	4	8	8	3	4

*E Foam (blended polymeric/rubber compound used as thermal insulation); Sh Fl 1 (commercial PVC floor covering, with inorganic felt backing); Fl Tile (commercial filled PVC floor tile); PP Crp (carpet with polypropylene yarn and scrim); Lens (polymeric material used to cover fluorescent light fixtures); Sh Fl 2 (residential unfilled PVC floor covering); AVG (average); STD (standard deviation); CV% (coefficient of variance).

Appendix C Interlaboratory Application

This appendix is not a part of the requirements of this NFPA document but is included for informational purposes only.

C-1 Calibration of the Working Heat Flux Meter. The calibration of the heat flux meter should be checked, whenever a recalibration of the apparatus is carried out, by comparison with two instruments of the same type as the working heat flux meter and of similar range, held as reference standards and not used for any other purpose. One of the heat flux meter reference standards should be fully calibrated at an accredited laboratory at yearly intervals. This meter should be used to calibrate the heater temperature controller. [See Figures 2-3.2 (a) and 2-3.2 (b).] It should be positioned at a location equivalent to the center of the specimen face during this calibration. One option for making the intercomparison of working and reference standard heat flux meters required in 2-3.4.3 is the use of the conical heater (see 2-3.1), with each heat flux meter mounted in turn in the calibration position (see 2-3.1.2), with care being taken to allow the whole apparatus to attain thermal equilibrium. Alternatively, use an apparatus specially built for comparative purposes — for example, as described in BS 6809, *Method of Calibration of Radiometers for Use in Fire Testing*.

It is noted that the use of two reference standards rather than one provides a greater safeguard against change in sensitivity of the reference instruments.

C-2 Variability in the Specific Optical Density of Smoke Measured in this Single Chamber Test.

C-2.1 A preliminary interlaboratory trial has been carried out in which replicate batches of sixteen materials were tested in accordance with this test method by eight laboratories (in six countries). This preliminary interlaboratory trial showed that

the specific optical densities D_s (at 10 minutes) of some materials had a higher relative variability than those of others. The relative variability increased particularly for those materials that did not ignite readily at an incident heat flux of 25 kW/m², and for those materials that showed higher D_s (at 10 minutes) values in the nonflaming mode than in the flaming mode.

C-2.2 The preliminary interlaboratory trial has demonstrated the ability of this test apparatus to discriminate between materials that generate different levels of smoke. Tables B-1(a) and B-1(b) present the repeatabilities and reproducibilities of D_s (at 10 minutes) for five plastics and five building materials, as derived in accordance with the statistical analysis in ISO 5725, *Precision of Test Methods — Determination of Repeatability and Reproducibility for Standard Test Method by Interlaboratory Tests*.

C-2.3 Repeatability, r , is the value below which the difference between two D_s (at 10 minutes) values obtained with the same method on identical test samples, under the same conditions (same laboratory, same apparatus, same operator, within a short interval of time), might be expected to lie with a 95 percent probability.

C-2.4 Reproducibility, R , is the value below which the difference between two D_s (at 10 minutes) values obtained with the same method on an identical test sample, under different conditions (different laboratories, different operators, different apparatuses), might be expected to lie with a 95 percent probability.

C-2.5 The preliminary interlaboratory trial has suggested that it is not meaningful to quote a single value for the variability of the test. The D_s (at 10 minutes) data show that smoke generation depends on the ignition behavior of the materials

(among other factors). Since ignition times are sensitive to irradiance (or incident heat flux), it is clear that careful attention should be paid to the measurement of irradiance.

C-2.6 A further examination of repeatability was also conducted in a single laboratory for wood samples, and the results are shown in Table B-1 (c). It is clear from these results that the repeatability of the test method is much better if the materials tested undergo consistent ignition under the conditions used for testing.

C-2.7 Six different products were selected for evaluation in a single laboratory. These selections represent typical commercial products that display a wide range of responses when subjected to the heat fluxes and the ignition source employed in this test method. An analysis of the data was conducted as a measure of the repeatability of the test method. See Table B-1 (d), which also identifies the products included in the study. The repeatability of the test method for this selection of products is good, as indicated by the calculated coefficient of variance, *CV*%. Some of the products are difficult to ignite, some of them bulge toward the heater, and some of them melt; however, the combination of the cone heater and the horizontal orientation minimizes the effect of these common performance problems.

Appendix D Determination of Mass Optical Density (MOD)

This appendix is not a part of the requirements of this NFPA document but is included for informational purposes only.

D-1 Introduction. The values of mass optical density determined by this test method are specific to the specimen used in the form and thickness tested and are not to be considered inherent or fundamental properties.

D-1.1 Principles of the Test. The conditions of thermal exposure and of smoke collection are the same as those in the mandatory part of the test method. Additional mass loss measurements are conducted on the specimen during the test, so that a mass loss/time curve is determined and mass optical density can then be calculated.

D-1.2 Test Specimen. The same specifications on suitability of materials, products, or assemblies apply here as in the mandatory portion of the test method. (See Chapter 4.) Similarly, the same number of specimens, their preparation, and their conditioning also applies. (See Chapter 5.)

D-1.3 Ancillary Equipment.

D-1.3.1 The load cell should have a measuring range of 500 g, and a weighing accuracy of ± 0.1 g. Mount the load cell in an enclosure [see Figures D-1.3.1(a), D-1.3.1(b), D-1.3.1(c), and D-1.3.1(d)] with a close-fitting labyrinth seal between the sample support rod and the enclosure, to minimize ingress of smoke particles and aggressive combustion products.

D-1.3.2 To level the unit on the base plate, the load cell enclosure should be fitted with one fixed foot and two adjustable feet. The load cell should also have a means to centralize the load cell assembly beneath the cone radiator.

D-1.3.3 The load cell should have a safe operating temperature range of 15°C to 70°C. A mineral fiberboard shield should be positioned over the top and sides of the load cell

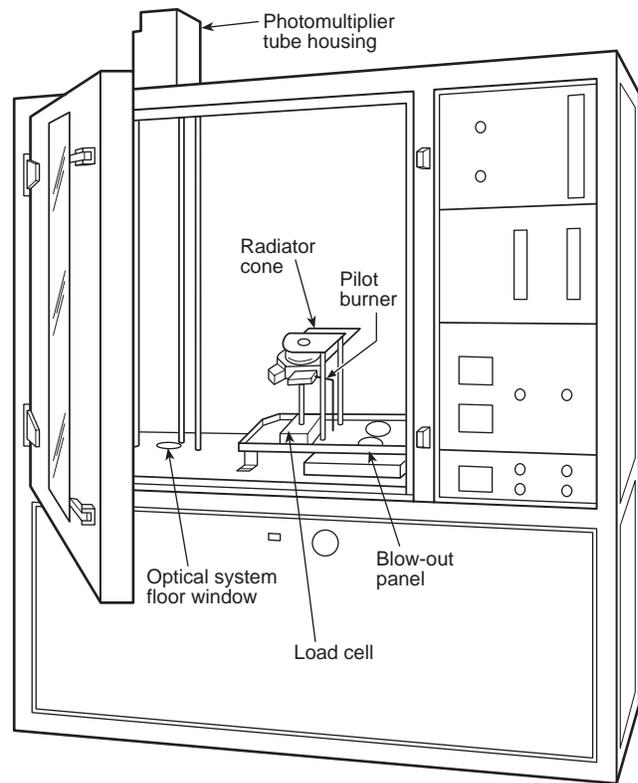


Figure D-1.3.1(a) Typical arrangement of test chamber with load cell.

enclosure during thermal exposure of the test specimen so that excessive temperature rise within the enclosure is prevented and drift of the load cell is avoided.

D-1.3.4 The load cell should be connected to a controller that drives the load cell and that is situated externally to the smoke chamber.

This controller should preferably be fitted with a digital mass display, a scaleable millivolt output, and a sample tare facility.

D-1.4 Calibration Procedures. The load cell calibration shall be checked with standard reference weights, in the range of test specimen mass, before each series of tests.

D-1.5 Test Procedure. Conduct the test in the same manner as detailed in Chapter 7, with the added precaution of ensuring that the load cell measurements are conducted properly.

D-1.6 Calculation of Mass Optical Density (MOD). For each specimen, calculate the mass optical density (in m^2/kg) at 10 minutes using the following equation:

$$MOD = \left(\frac{D}{L}\right)\left(\frac{V}{D_m \times 0.001}\right)$$

where:

D = optical density of smoke

L = length of light path

V = volume of the chamber

D_m = mass loss of the test specimen ($D_m = m_i - m_f$) in g